



## INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

(51) International Patent Classification <sup>6</sup> : A61B 17/00	A1	(11) International Publication Number: <b>WO 97/33520</b> (43) International Publication Date: 18 September 1997 (18.09.97)
---	----	--

(21) International Application Number: PCT/US97/04210

(22) International Filing Date: 12 March 1997 (12.03.97)

## (30) Priority Data:

08/615,151	12 March 1996 (12.03.96)	US
08/672,164	27 June 1996 (27.06.96)	US

(71) Applicant: HEARTPORT, INC. [US/US]; 200 Chesapeake Drive, Redwood City, CA 94063 (US).

(72) Inventors: FLOM, James, R.; 2557 Park Boulevard, L102, Palo Alto, CA 94306 (US). RAY, Pinaki; 1309 Marshall Street #305, Redwood City, CA 94063 (US). GIFFORD, Hanson, S., III; 3180 Woodside Road, Woodside, CA 94062 (US). HOEKENDIJK, Jens, E.; 601 Corbett Street, San Francisco, CA 94114 (US).

(74) Agents: HESLIN, James, M. et al.; Townsend and Townsend and Crew L.L.P., 8th floor, Two Embarcadero Center, San Francisco, CA 94111-3834 (US).

(81) Designated States: AU, CA, JP, European patent (AT, BE, CH, DE, DK, ES, FI, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).


**Published**

*With international search report.  
Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.*

(54) Title: IMPROVED TROCAR

## (57) Abstract

The invention is a thoracic trocar having a deflectable member (12, 17). The deflectable member has a frustoconical outer surface and is movable between first and second positions. The outer surface is angled toward the distal end in the first position and angled toward the proximal end in the second position. The first and second positions are both stable, unbiased positions and the deflectable member is movable from the first position to the second position upon application of the necessary force.

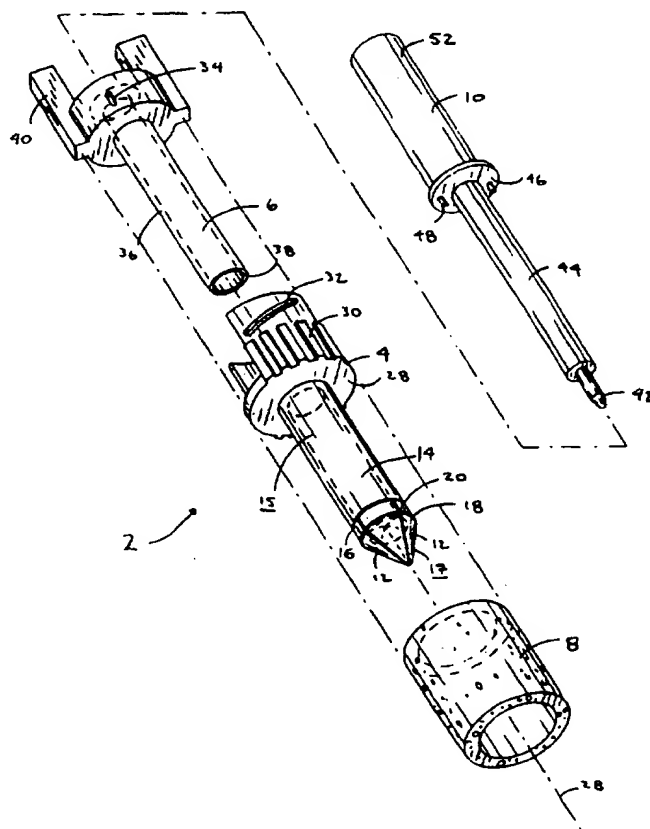

**FOR THE PURPOSES OF INFORMATION ONLY**

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AM	Armenia	GB	United Kingdom	MW	Malawi
AT	Austria	GE	Georgia	MX	Mexico
AU	Australia	GN	Guinea	NE	Niger
BB	Barbados	GR	Greece	NL	Netherlands
BE	Belgium	HU	Hungary	NO	Norway
BF	Burkina Faso	IE	Ireland	NZ	New Zealand
BG	Bulgaria	IT	Italy	PL	Poland
BJ	Benin	JP	Japan	PT	Portugal
BR	Brazil	KE	Kenya	RO	Romania
BY	Belarus	KG	Kyrgyzstan	RU	Russian Federation
CA	Canada	KP	Democratic People's Republic of Korea	SD	Sudan
CF	Central African Republic	KR	Republic of Korea	SE	Sweden
CG	Congo	KZ	Kazakhstan	SG	Singapore
CH	Switzerland	LI	Liechtenstein	SI	Slovenia
CI	Côte d'Ivoire	LK	Sri Lanka	SK	Slovakia
CM	Cameroon	LR	Liberia	SN	Senegal
CN	China	LT	Lithuania	SZ	Swaziland
CS	Czechoslovakia	LU	Luxembourg	TD	Chad
CZ	Czech Republic	LV	Latvia	TG	Togo
DE	Germany	MC	Monaco	TJ	Tajikistan
DK	Denmark	MD	Republic of Moldova	TT	Trinidad and Tobago
EE	Estonia	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	UG	Uganda
FI	Finland	MN	Mongolia	US	United States of America
FR	France	MR	Mauritania	UZ	Uzbekistan
GA	Gabon			VN	Viet Nam

IMPROVED TROCAR

## FIELD OF THE INVENTION

The present invention relates to trocars and their methods of use. A specific application of the trocar is developed with respect to use in a patient's thoracic cavity, however, the trocars may be used for any other purpose. The trocars provide a path for surgical instruments into a patient.

## BACKGROUND OF THE INVENTION

Trocars are generally used as access devices for introduction of other surgical instruments into a patient. A conventional thoracic trocar is disclosed in U.S. Patent No. 5,279,575 to Sugarbaker. In U.S. Patent No. 5,279,575 the trocar has a pair of flukes which are pivotally coupled to the body with pins. The trocar also includes a rigid clamp which is slidably on the outer tube for securing the trocar to a body wall. The inner tube slides longitudinally relative to the outer tube for moving the flukes to the open position. A distal end of the inner tube engages a camming surface on each of the flukes for camming the flukes outward,

The trocar disclosed in U.S. Patent No. 5,279,575 suffers from a number of drawbacks. First, the clamp is relatively stiff and does not conform to the shape of the patient. As such, the trocar may be difficult to tilt at a desired angle when passing between adjacent ribs. Another drawback of the trocar is that the hinges create a relatively large profile since the hinges extend beyond the outer, cylindrical surface of the tube. The relatively large profile increases trauma to the patient which is particularly problematic when the trocar is rotated or otherwise displaced after initial placement. Yet another drawback of U.S. Patent

No. 5,279,575 is that the clamp is mounted to a third tube which slides over the outer tube. The three tube configuration also increases the profile of the device and trauma to the patient.

#### SUMMARY OF THE INVENTION

The present invention solves the problems with known trocars by providing a trocar body having arms which lie within a cylinder defined by the trocar body. The arms are positioned within the cylinder when in the closed position so that the profile of the trocar is minimized. The arms are preferably integrally formed with the tubular portion. An actuator is positioned within the body and movable with respect to the body in a longitudinal direction. The actuator slidably engages the arms for moving the arms from the closed position to the open position. In a preferred embodiment, the actuator is rotatably coupled to the body by a pin and slot configuration. Rotation of the actuator moves the distal end of the actuator longitudinally to engage the arms for moving the arms to the open position.

The trocar also preferably includes a resilient member attached to the body. The resilient member is configured to provide a clamping force on tissue positioned between the arms and the resilient member when the arms are in the closed position. The resilient member provides advantages over conventional clamps since the resilient member conforms to the shape of the patient.

In another aspect of the present invention, a trocar is provided with a deflectable member coupled to the distal end of an outer member. The deflectable member has first and second ends with the first end coupled to an inner member. The inner member is rotatably coupled to the outer member for moving the first end between open and closed positions. When the first end is in the open position the deflectable member is deflected outwardly for locking the trocar to a patient. The first end travels along an arcuate path when moving between the open and closed position. In a preferred embodiment, the inner and outer members are substantially

cylindrical and the deflectable member is integrally formed with the outer member.

In yet another aspect of the present invention, a trocar includes an inner member and an outer member surrounding at least a portion of the inner member. The inner member includes arms which are movable between closed and open positions. The arms are configured to lock the trocar to a patient when in the open position. The outer member is attached to the arms for moving the arms to the open position. The outer member is moved longitudinally relative to the inner member to move the arms to the open position.

In another aspect of the present invention, a trocar includes an inner member having arms at a distal end. The arms are biased toward an open position and are restrained in the closed position by an outer member which engages an outer surface of the arms. When the outer member is retracted, the outer member is spaced apart from the outer surface of the arms which permits the arms to move to the open position. In a preferred embodiment, the outer member is substantially cylindrical and slidably engages the inner member when moving the arms to the closed position.

In yet another aspect of the present invention, a trocar includes arms which have interlocking elements. The interlocking elements hold the arms in a closed position. The interlocking elements are preferably hooks which are deflected to disengage from one another when an instrument is inserted through the trocar. The arms are naturally biased toward the open position so that the arms move to the open position when the hooks disengage.

In another aspect of the present invention, a trocar is provided which includes a deflectable member. The deflectable member is movable between first and second positions with both the first and second positions being stable, unbiased positions. The deflectable member preferably has a frustoconical shape which is angled toward the distal end in the first position and toward the proximal end in the second position. The trocar is inserted into the patient with the deflectable member in the first position to facilitate

introduction into the patient. When it is desired to remove the trocar, the trocar is pulled with sufficient force to move the deflectable to the second position for removal of the trocar from the patient.

5           These and other features will become apparent with the following description of the preferred embodiments.

#### BRIEF DESCRIPTION OF THE DRAWINGS

Fig. 1 is an exploded view of a first trocar.

10           Fig. 2 is a cross-sectional view of the first trocar with arms in a closed position.

Fig. 3 is a cross-sectional view of the first trocar with the arms in an open position.

Fig. 4 is an isometric view of a second trocar.

15           Fig. 5 is a side view of the second trocar with an adhesive strip adhering the second trocar to the patient.

Fig. 6 is an isometric view of a third trocar.

Fig. 7 is a cross-sectional view of the third trocar with arms in a closed position.

20           Fig. 8 is an isometric view of the third trocar with the arms in an open position.

Fig. 9 is a cross-sectional view of the third trocar with the arm in a closed position.

25           Fig. 10 is an isometric view of a fourth trocar with arms in an open position.

Fig. 11 is an isometric view of the fourth trocar with the arms in a closed position.

Fig. 12 is a partial cut-away plan view of the fourth trocar with the arms in the closed position.

30           Fig. 13 is another partial cut-away plan view of the fourth trocar with the arms in the open position.

Fig. 14 is an isometric view of a fifth trocar with arms in a closed position.

35           Fig. 15 is an isometric view of a fifth trocar with arms in the open position.

Fig. 16 is a view of the bottom of the fifth trocar.

Fig. 17 is an isometric view of a sixth trocar.

Fig. 18 is a partial cross-sectional view of the sixth trocar of Fig. 17.

Fig. 19 is a side view of a seventh trocar.

Fig. 20 is a cross-sectional view of the seventh trocar with a deflectable member in a first position.

Fig. 21 is a cross-sectional view of the seventh trocar with the deflectable member in a second position.

#### DESCRIPTION OF THE PREFERRED EMBODIMENT

Referring to Fig. 1, a trocar 2 constructed in accordance with the present invention is shown. The trocar 2 includes a body 4, an actuator 6, a resilient member 8, and an obturator 10 which is optional. The body 4 includes a number of arms 12 which are movable from the closed position of Fig. 2 to the open position of Fig. 3. As will be described below, the actuator 6 is used to move the arms 12 from the closed position of Fig. 2 to the open position of Fig. 3.

Referring now to Figs. 1 and 2, the body 4 includes a tubular portion 14 having an exterior surface 15 which defines a cylinder. The arms 12 of the present invention advantageously do not extend outside the cylinder defined by the external surface 15 of the tubular portion 14 so that trauma to a patient is minimized. The small profile of the trocar 2 is accomplished by forming the arms 12 integrally with the tubular portion 14.

The arms 12 preferably form a tip and form an outer surface 17 having a conical or frustoconical shape. A notch 16 is provided where the arms 12 bend when moving from the closed position to the open position. The arms 12 are preferably biased toward the closed position by an o-ring 18 positioned in a groove 20. Referring to Figs. 2 and 3, the arms 12 each include a slide surface 22 which is engaged by the actuator 6 when moving the arms 12 from the closed position to the open position. The slide surface 22 is oriented substantially perpendicular to a longitudinal axis 26, however, the slide surface 22 may also have any other orientation including curved to facilitate deflection of the arms 12 from the closed position to the open position. The

arms 12 are moved from the closed position to the open position by the actuator 6 as will be described below.

A flange 28 is connected to the proximal end of the tubular portion 14. The flange 28 includes ribs 30 and an arcuate slot 32. The slot 32 receives a pin 34 attached to the actuator 6. The pin 34 and slot 32 configuration produces a longitudinal displacement of the actuator 6 relative to the arms 12 when the actuator 6 is rotated relative to the body 4.

The actuator 6 includes a member 36, which is preferably a cylindrical tube, having a distal end 38 which contacts and engages the slide surface 22 for moving the arms 12 to the open position. The actuator 6 also includes a pair of extensions 40 which are grasped by the user for rotating the actuator 6 relative to the body 4.

The resilient member 8 is preferably cylindrical with an annular cross-sectional shape. A preferred material for the resilient member 8 is polyurethane foam although any resilient material may be used. The resilient member 8 is preferably spaced apart from the tubular portion 14 which facilitates angling the trocar 2 when the trocar 2 is positioned between adjacent ribs. The space between the resilient member 8 and tubular portion 14 permits radial deflections of the resilient member 8 to facilitate angling of the trocar 2. The resilient member 8 is preferably attached to the flange 28 with an adhesive. Another advantage of the resilient member 8 is that it conforms to the patient thereby reducing trauma to the patient. A further advantage of the resilient member 8 is that it does not require manipulation of set screws and the like as is required with the trocar of U.S. Patent No. 5,279,575.

Referring to Fig. 2, the obturator 10, which is optional, has a tip 42 which extends beyond the distal tip of the arms 12. Alternatively, the obturator 10 may be omitted with the arms 12 forming the tip as shown in Fig. 1. The tip 42 of the obturator 10 is preferably rounded to reduce trauma to the patient when the trocar 2 is inserted into the patient. The obturator 10 includes a shaft 44 and a flange 46 having a pair of pins 48 which engage holes 50 in the actuator 6. The



proximal end has a handle 52 for manipulating the obturator 10. The obturator 10 may also be used to rotate the actuator 6 by rotating the handle with the pins 48 engaging the holes 50 in the actuator 6.

5           Use of the trocar 2 is now described with reference to Figs. 2 and 3. Referring to Fig. 2, the arms 12 are shown in the closed position. The o-ring 18 biases the arms 12 toward the closed position. When using the trocar 2 to access the thoracic cavity, a hole is formed between adjacent ribs in the patient and the trocar 2 is inserted into the hole with the arms 12 in the closed position. Referring to Fig. 3, the actuator 6 is then rotated in the direction of arrow A. The pin 34 engages the slot 32 and moves the actuator 6 longitudinally in the direction of arrow B. The distal end of the actuator 6 engages the slide surface 22 thereby deflecting the arms 12 to the open position. With the obturator 10 removed, the throughhole may be used for the introduction of surgical instruments into the patient's thoracic cavity. When the trocar 2 is used in the thoracic cavity, the arms 12 engage the thoracic wall and the resilient member 8 engages the patient's chest. The resilient member 8 is compressed thereby providing a clamping action on the body cavity wall between the resilient member 8 and the arms 12 to anchor the trocar 2. The clamping action secures the trocar 2 to the body wall and minimizes the length of the trocar 2 extending beyond the body wall and into the patient.

Referring to Figs. 4 and 5, a second trocar A is shown. The trocar A is the same as trocar 2 with the exception that the resilient member 8 is replaced by a number of adhesive strips 54 with like reference numerals referring to like structure. The adhesive strips 54 are used to anchor the trocar A to the patient. An advantage of the adhesive strips 54 is that when the trocar A is angled with respect to the outer surface of the patient, the adhesive strips 54 may be used in the appropriate location to maintain the angular orientation.

A removable cover 56 covers each of the adhesive strips 54. The cover 56 has a pull tab 57 extending outwardly

from the flange 28. The cover 56 doubles back upon itself so that an end 59 of the cover 56 is also positioned near the flange 28. The cover 56 may, of course, be simply a strip of material which terminates at the distal end or which has a perforated end which tears away from the body 4. After the cover 56 has been removed, a tab 58 on the adhesive strip 54 is pulled so that the adhesive strip 54 tears away from the body 4. An adhesive side 60 is then adhered to the patient's skin. Referring to Fig. 5, the arms 12 are in the open position to engage an inner thoracic wall. If the trocar A is removed from the patient, the adhesive strip 54 is preferably torn away completely from the body 4. If the trocar A is inserted into the patient again, another one of the adhesive strips 54 is used to secure the trocar A to the patient.

Referring to Figs. 6 and 7, a third preferred trocar 2d is shown. The trocar 2d includes an inner member 62 which extends through an outer member 64. The inner member 62 includes a throughhole 66 for introduction of medical instruments into a patient.

A number of arms 63 are integrally formed with a tubular portion 68 of the inner member 62. Although it is preferred that the arms 63 are integrally formed with the tubular portion 68, the arms 63 may also be pivotally coupled to the tubular portion 68 with a pinned connection. The arms 63 are naturally biased toward the closed position of Fig. 6, however, the trocar 2d may also include the groove and o-ring of Fig. 1 and 2.

The outer member 64 has a distal end 70 which is coupled to the arms 63. The outer member 64 has a rigid cylindrical portion 72 and an elastomeric portion 74 which has the distal end 70 attached to the arms 63. The distal end 70 of the outer member 64 has a number of slots 76 therein which form a number of sections 78 corresponding to the arms 63 with each of the sections 78 being connected to one of the arms 63.

The outer member 64 is rigidly coupled to a ring 80 and a resilient member 8 is attached to the ring 80. The resilient member 8 is preferably the same as the resilient

member 8 described above in connection with Figs. 1 and 2. The ring 80 includes a curved slot 82 which receives a pin 84 attached to a lever 86. The other end of the lever 86 is pinned to an extension 88 of the inner member 62.

5 Referring to Figs. 8 and 9, pivoting of the lever 86 in the direction of arrow C moves the inner member 62 longitudinally relative to the outer member 64. The relative motion causes the outer member 64 to go into tension so that the outer member pulls the arms 63 to the open position of  
10 Figs. 8 and 9. Although it is preferred to use the lever 86 to produce relative longitudinal displacement between the inner and outer members 62, 64, the inner and outer members 62, 64 may also be simply slidable relative to one another or have the pin and slot configuration of Figs. 1 and 2.

15 Referring to Figs. 10 and 11, a fourth preferred trocar 2d is shown. The trocar 2d includes an inner member 90 rotatably coupled to an outer member 92. Arms 94 are mounted to the outer member. The arms 94 are movable from the closed position of Fig. 10 to the open position of Fig. 11.  
20 As will be described below, the arms 94 are moved from the closed position to the open position by relative rotational motion between the inner and outer members 90, 92. The inner and outer members 90, 92 may take any shape, however, a preferred shape is cylindrical. A through hole 96 extends  
25 through the trocar 2d for the introduction of surgical instruments.

The arms 94 are preferably formed by making two L-shaped cuts in the distal end of the outer member 92. The arms 94 each include a first end 98, which is coupled to the  
30 outer member 92, and a second end 100, which is attached to the inner member 90. The first end 98 is preferably integrally formed with the outer member 92. The outer member 92 is coupled to a ring 104 and a resilient member 8 is attached to the ring 104. The resilient member 8 is  
35 preferably the same as described above and serves the same purpose. Although it is preferred to use the resilient member 8, a conventional clamp may be also be used such as the clamp disclosed in U.S. Patent No. 5,279,575

The inner member 90 is coupled to a driver 106. When the driver 106 is rotated in the direction of arrow D the second end 100 travels along an arcuate path toward the first end 98. The arcuate path preferably lies in a plane which is substantially perpendicular to a longitudinal axis 108 of the inner member 90. The arcuate path may be oriented in any other configuration relative to the longitudinal axis 108 and preferably forms an angle of between 90° and 45° with the longitudinal axis 108.

Figs. 12 and 13 are partial cut-away showing the arms 94 in the closed and open positions, respectively. Although it is preferred to provide two arms 94, any number of arms 94 may be provided. The arms 94 are preferably both positioned at the same longitudinal position, however, the arms 94 may also be positioned at different locations along the longitudinal axis. Furthermore, the arms 94 may include a hinge between the first and second ends 98, 100 to form a predetermined shape.

The inner and outer members 90, 92 may be locked in the open and closed positions. Referring to Fig. 10 and 11, an extension 110 extends from the ring 104. The extension 110 has a protrusion 112 which is configured to engage detents 114 in the driver 106. The driver 106 includes a cut-out 115 in which the extension 110 is positioned. The actuator 6 is locked and unlocked by twisting the driver 106 with a sufficient force to deflect the extension 110 so that the protrusion 112 engages or disengages from the detent 114.

Referring to Figs. 14-16, a fifth trocar 2D is shown. The trocar 2D includes a number of arms 116 which have interlocking elements 118 which, in the preferred embodiment, are hooks. Referring to the end view of Fig. 16, the interlocking elements 118 engage one another to retain the arms 116 in the closed position of Fig. 14. The arms 116 are naturally biased toward the open position of Fig. 15 and the interlocking elements 118 retain the arms 116 in the closed position of Fig. 14. The arms 116 are preferably integrally formed with a tubular portion 120. The trocar 2D includes a

through hole 122 for introduction of surgical devices into the patient.

Referring to Fig. 15, the arms 116 include slide surfaces 124. The interlocking elements 118 are disengaged from one another by inserting an instrument into the throughhole 122 to engage the slide surfaces 124. The instrument deflects the interlocking elements 118 until they become disengaged from one another. After the interlocking elements 118 are disengaged, the arms 116 move to their natural, unbiased, position of Fig. 15. The trocar 2D also includes the resilient member 8, however, a conventional clamp may also be used. Although it is preferred to use hooks as the interlocking elements 118, the interlocking elements 118 may have any other structure. For example, the interlocking elements 118 may be an adhesive or a frangible connection which could be machined or formed by melting the arms 116 together and which is broken by the instrument. Alternatively, the connection may be melted or broken by a heated instrument. Furthermore, although it is preferred that the interlocking elements 118 be disengaged with any medical instrument, a specialized opener may be used which engages the arms 116. The specialized instrument could include teeth which engage teeth on the arms 116 so that a rotational action is used to disengage the interlocking elements 118. The specialized instrument may also be used to hold the arms in the closed position and is simply removed to permit the arms to move to the unbiased, open position.

Referring to Figs. 17 and 18, a sixth preferred trocar is shown. The trocar Be includes an inner member 126 having a number of arms 128 at a distal end 130. The arms 128 are naturally biased to the open position of Fig. 18 and are maintained in the closed position of Fig. 17 by an outer member 130. The outer member 130 has a cylindrical portion 132 connected to a disc 134. The trocar Be preferably includes the resilient member 8, however, a conventional clamp may also be used.

The inner member 126 includes a pin 136 which engages a slot 138 in the outer member 130. Rotation of the

disc 124 causes the outer member 130 to displace longitudinally in the direction of arrow E. The distal end of the outer member 130, which restrains the arms 128 in the closed position of Fig. 17, is spaced from the arms 128 thereby permitting the arms 128 to move to the unbiased, open position of Fig. 18. The arms 128 are preferably integrally formed with the inner member 126 and are preferably made of a polyolefin plastic although any suitable material may be used. To remove the trocar Be, the disc 134 is rotated so that the distal end of the outer member 130 forces the arms 128 to the closed position of Fig. 10. The trocar Be is then removed from the patient. Alternatively, the trocar Be may be simply pulled from the patient with the body wall deflecting the arms 128 inward as they pass through the body wall.

Referring to Fig. 19, a seventh trocar 2F is shown which includes a deflectable member 150. An obturator 152 extends through the trocar 2F beyond a distal end 154 of the trocar 2F. The deflectable member 150 has an outer surface 156 which preferably has a frustoconical shape. The deflectable member 150 also has an inner surface which is spaced apart from the wall so that the deflectable member 150 may be deformed when inserted into the patient.

The deflectable member 150 is shown in a first position in Fig. 19 with the outer surface 156 being angled toward the distal end 154. Referring to the cross-sectional view of Fig. 21, the deflectable member 150 is shown in the second position in which the outer surface 156 is angled toward the proximal end. The outer surface 156 and inner surface of the deflectable member 150 are everted when moving from the first position to the second position. The deflectable member 156 preferably moves from the first position to the second position upon application of an axial force of between 2 and 5 lbs and more preferably between 3 and 4 lbs.

Referring to Fig. 20, the deflectable member 150 is integrally formed with an elastomeric sheath 158. The sheath 158 is made of silicone rubber however, any other suitable elastic material may be used. The deflectable member 150 has

a hinge 160 which is stable in both the first position of Fig. 20 and the second position of Fig. 21. The sheath 158 includes a helical thread 162 so that the user may also rotate the trocar 2F to position the trocar 2F in the chest wall or other body structure. The thread 162 also helps prevent inadvertent removal of the trocar 2F. The trocar 2F may, of course, be formed without the helical thread 162 or with circumferential ribs if desired. An instrument delivery lumen 164 passes through the trocar 2F for introducing surgical instruments into a patient. The instrument delivery lumen 164 may also include gas seals if a gas, such as carbon dioxide, is introduced and retained into the patient.

The sheath 158 is mounted to an inner cannula 166 which is made of a low friction plastic so that surgical instruments pass easily through the instrument delivery lumen 164 without binding. The sheath 158 may either be attached to the inner cannula 166 with an interference fit or with an adhesive. The inner cannula 166 and sheath 158 could also be con-injection molded to provide a single cannula with the sheath 158 being an elastomer and the inner cannula 156 being a low friction plastic. A distal end of the inner cannula 166 has a beveled edge 168 and extends beyond the sheath 158. The beveled edge 168 provides a smooth transition between the obturator 152 and trocar 2F. The beveled edge 168 also provides a smooth transition between the inner cannula 166 and deflectable member 150.

The inner cannula 166 has a flange 170 at the proximal end. A clamp 172 is mounted to the bottom of the flange 170 to provide a clamping force on a body structure positioned between the clamp 172 and the deflectable member 150. The clamp is also used to retract the distal end of the trocar 2F so that the deflectable member 150 engages a body structure such as the thoracic wall. The clamp 172 is preferably the same as the resilient member 8 described above in connection with Figs 1-3, however, any other clamp may be used such as a coil spring.

The above description merely describes the preferred embodiments and it is understood that variations of the

5 preferred embodiment are within the scope of the invention which is defined by the claims. For example, the trocar 2D may include the outer member 130 to move the arms 12 to the closed position after the interlocking members 118 have been disengaged, and the obturator 10 may be used with any of the trocars described herein.



WHAT IS CLAIMED IS:

1           1. A device used for introducing a surgical  
2 instrument into a patient, comprising:  
3           a body having a proximal end and a distal end;  
4           an instrument delivery lumen extending through the  
5 body; and  
6           a deflectable member coupled to the body, the  
7 deflectable member being made of an elastomeric material, the  
8 deflectable member having an outer surface which is angled  
1 toward the distal end of the body.

1           2. The device of claim 1, wherein:  
2           the outer surface has a frustoconical shape.

1           3. The device of claim 1, wherein:  
2           the body includes an elastomeric sheath; and  
3           the deflectable member being integrally formed with  
4 the elastomeric sheath.

5           4. A device used for introducing a surgical  
6 instrument into a patient, comprising:  
7           a body having a proximal end and a distal end;  
8           an instrument delivery lumen extending through the  
9 body; and  
10           a deflectable member coupled to the body, the  
11 deflectable member being movable between a first position and  
12 a second position, the first and second positions both being  
13 unbiased positions, the deflectable member being movable from  
14 the first position to the second position upon application of  
15 a force to the deflectable member.

1           5. The device of claim 4, wherein:  
2           the deflectable member includes an outer surface  
3 which is angled toward the distal end when the deflectable  
4 member is in the first position and which is angled toward the  
5 proximal end when the deflectable member is in the second  
6 position.

1           6.    The device of claim 4, wherein:  
2           the body includes an elastomeric sheath; and  
3           the deflectable member being integrally formed with  
4   the elastomeric sheath.

1           7.    The device of claim 4, wherein:  
2           the body includes a helical thread on an exterior  
3   surface.

1           8.    A trocar adapted for introduction of medical  
2   instruments into a patient, comprising:  
3           a body having a through hole defining a longitudinal  
4   axis, the body also having at least two arms movable between a  
5   closed position and an open position, the at least two arms  
6   being configured to secure the body to a body wall of a  
7   patient when in the open position, the body including a  
8   cylindrical portion having an outer surface defining a  
9   cylinder, the body having a portion distal to the cylindrical  
10   portion, the portion including the at least two arms and being  
11   positioned substantially within the cylinder when in the  
12   closed position; and  
13           an actuator at least partially positioned within the  
14   body and being movable with respect to the body in the  
15   direction of the longitudinal axis, the actuator slidably  
16   engaging the at least two arms for moving said at least two  
17   arms from the closed position to the open position.

1           9.    The trocar of claim 8, wherein:  
2           the at least two arms are integrally formed with the  
3   cylindrical portion.

1           10.   The trocar of claim 8, wherein:  
2           the at least two arms are biased toward the closed  
3   position.

1           11. The trocar of claim 8, wherein:  
2           the actuator is rotatably coupled to the body, the  
3           actuator being rotatable with respect to the body between a  
4           first position and a second position, the actuator moving the  
5           at least two arms from the closed position to the open  
6           position when the actuator moves from the first position to  
7           the second position, the actuator also displacing toward the  
8           distal end when moving from the first position to the second  
9           position.

1           12. The trocar of claim 8, further comprising:  
2           an adhesive strip coupled to the body, a portion of  
3           the adhesive strip being removable from the body for adhering  
4           the strip to a patient.

1           13. A trocar adapted for introduction of medical  
2           instruments into a patient, comprising:  
3           a body having a through hole defining a longitudinal  
4           axis, the body also having at least two arms movable between a  
5           closed position and an open position; and  
6           an actuator at least partially positioned within the  
7           body, the actuator engaging the at least two arms for moving  
8           said at least two arms from the closed position to the open-  
9           position, the actuating element being rotatably coupled to the  
10          body, the actuator displacing along the longitudinal axis when  
11          the actuator is rotated with respect to the body.

1           14. The trocar of claim 13, wherein:  
2           at least one of the body and actuator includes a  
3           slot and an other of the body and the actuator includes a pin  
4           received in the slot.

1           15. The trocar of claim 13, further comprising:  
2           a resilient member coupled to the body, the  
3           resilient member being configured to provide a clamping force  
4           on a body wall positioned between the at least two arms and  
5           the resilient member when the at least two arms are in the  
6           open position.

7 16. The trocar of claim 13, wherein:

8 the at least two arms each include a slide surface;

9 and

10 ~~the actuator slidably engages the slide surfaces of~~

11 the at least two arms for moving the at least two arms from

12 the closed position to the open position.

1 17. The trocar of claim 13, wherein:

2 the at least two arms are biased toward the closed  
3 position.

1 18. A trocar adapted for introduction of medical  
2 instruments into a patient, comprising:

3 an outer member;

4 an arm coupled to the outer member, the arm having a  
5 first end and a second end, the first end being movable  
6 between a closed position and an open position, the arms being  
7 configured to secure the trocar to a body wall of a patient  
8 when the first end is in the open position, the first end  
9 traveling along a path when moving between the closed and open  
10 positions, the path having an arcuate segment; and

11 an inner member at least partially positioned within  
12 the outer member, the inner member being connected to the  
13 first end of the arm, the inner member being movably coupled  
14 to the outer member between a first position and a second  
15 position, the first end being in the closed position when the  
16 inner member is in the first position and the arms being in  
17 the open position when the inner member is in the second  
18 position.

1 19. The trocar of claim 18 wherein:

2 the inner member is rotatably coupled to the outer  
3 member; and

4 the path traveled by the first end when moving  
5 between the open and closed positions is entirely arcuate.

1           20. The trocar of claim 18 wherein:  
2           the path lies in a plane which is substantially  
3           perpendicular to the longitudinal axis.

1           21. The trocar of claim 18 wherein:  
2           the second end of the arm is integrally formed with  
3           the outer member.

1           22. A trocar adapted for introduction of medical  
2           instruments into a patient, comprising:  
3           an inner member having at least two arms movable  
4           between a closed position and an open position, the at least  
5           two arms being configured to secure the trocar to a body wall  
6           of a patient when in the open position, the inner member  
7           having a through hole for introduction of instruments into a  
8           patient; and

9           an outer member surrounding at least a portion of  
10          the inner member, the outer member being attached to the at  
11          least two arms, the outer member being movable along the  
12          longitudinal axis between a first position, in which the at  
13          least two arms are in the closed position, and a second  
14          position, in which the at least two arms are in the open  
15          position.

1           23. The trocar of claim 22, wherein:  
2           the at least two arms are biased toward the closed  
3           position.

1           24. A trocar adapted for introduction of medical  
2           instruments into a patient, comprising:

3           a first member having arms at a distal end, the arms  
4           being movable between a closed position and an open position,  
5           the arms being biased toward the open position, the arms being  
6           configured to secure the trocar to a body wall of a patient  
7           when in the open position; and

8           a second member surrounding at least a portion of  
9           the first member, the second member being movably coupled to  
10          the first member between a first position and a second

11 position, the second member engaging the outer surface of the  
12 arms for restraining said arms in the closed position when the  
13 second member is in the first position, the second member  
14 ~~being spaced apart from the outer surface of the arms when in~~  
15 the second position so that the arms are free to move to the  
16 open position.

1 25. The trocar of claim 24, wherein:

2 the second member has a substantially cylindrical  
3 distal end, the second member having an inner surface which  
4 engages the arms when the second member is in the first  
5 position.

1 26. The trocar of claim 24, wherein:

2 the second member slidably engages the first member  
3 when moving the arms to the closed position.


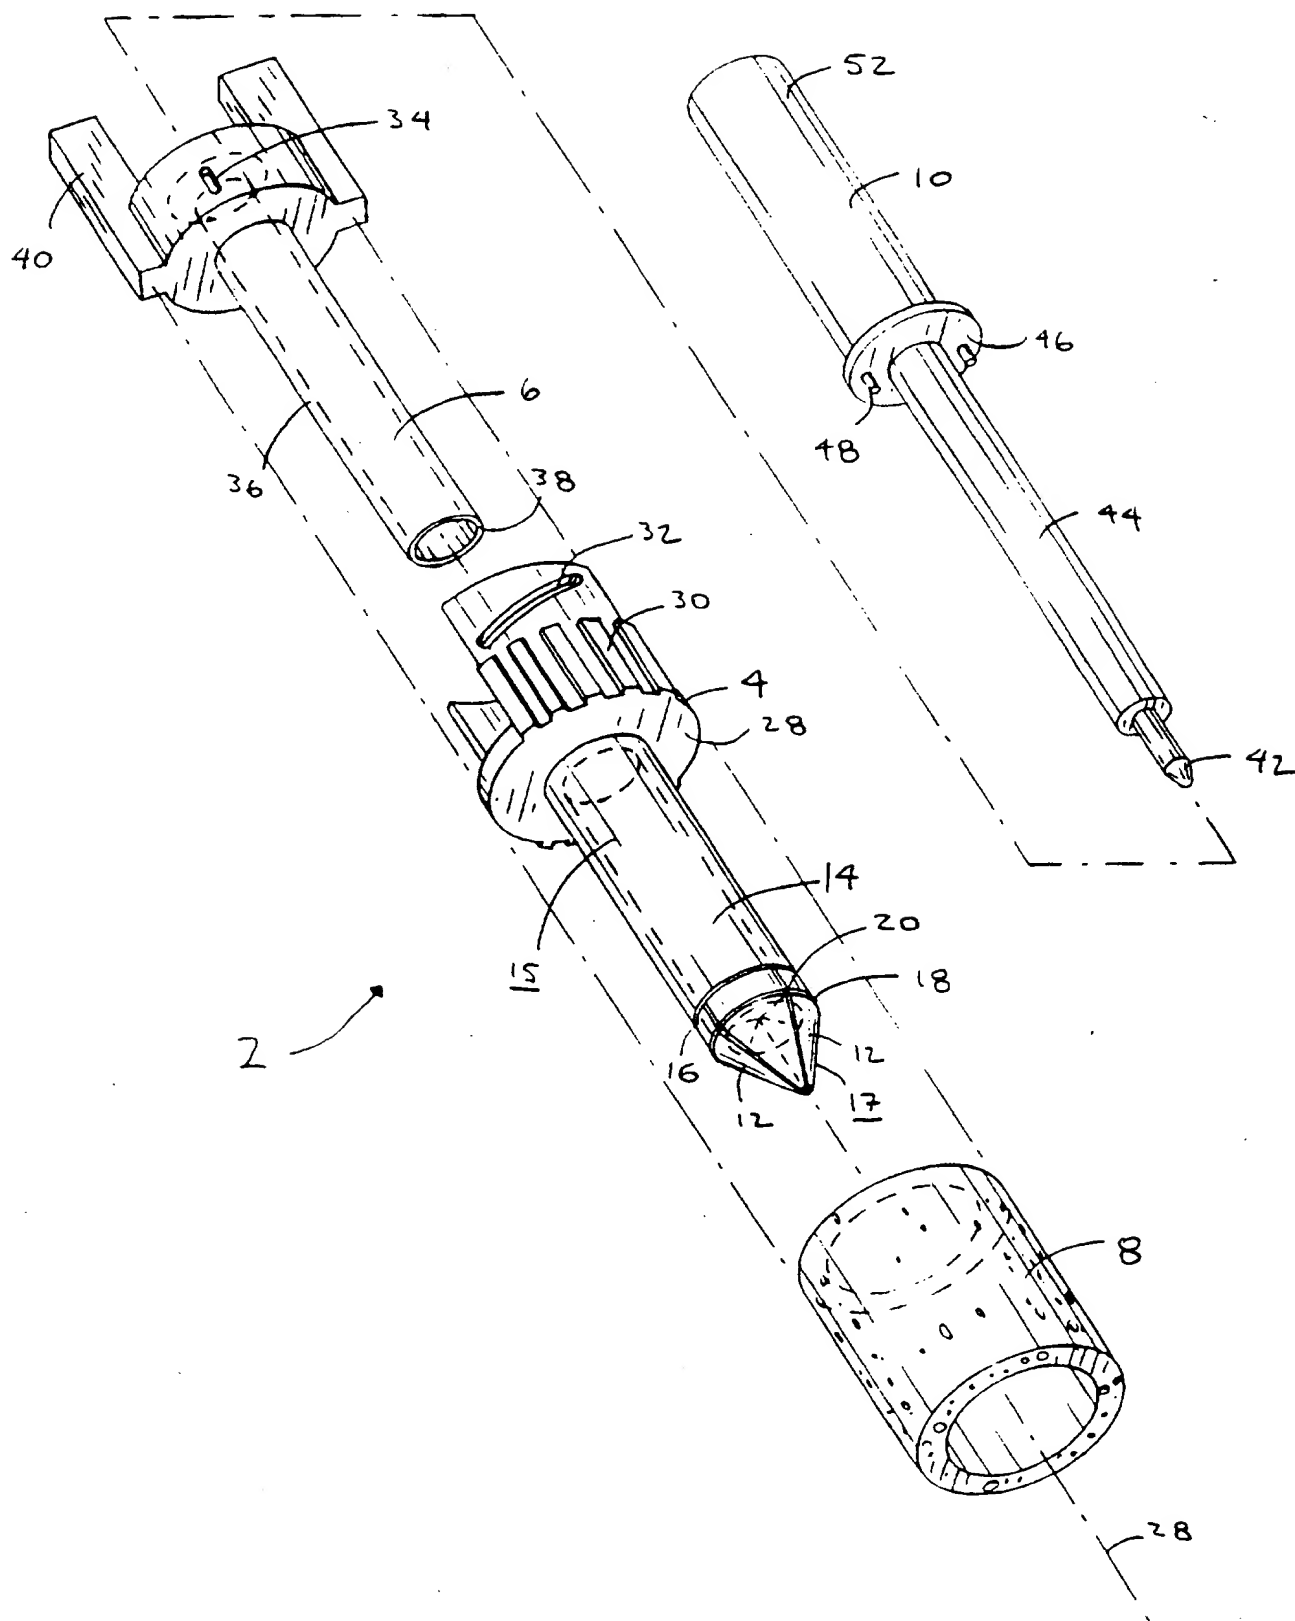


FIG. 1


2 / 11

**FIG. 2**

SUBSTITUTE SHEET (RULE 26)

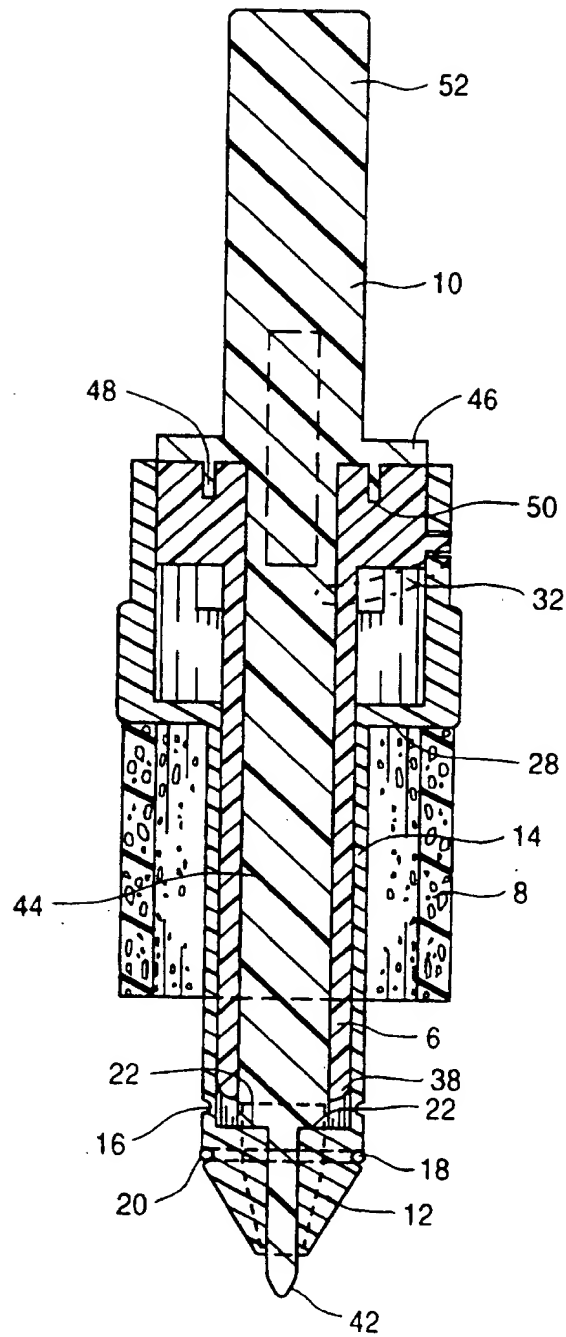

3 / 11

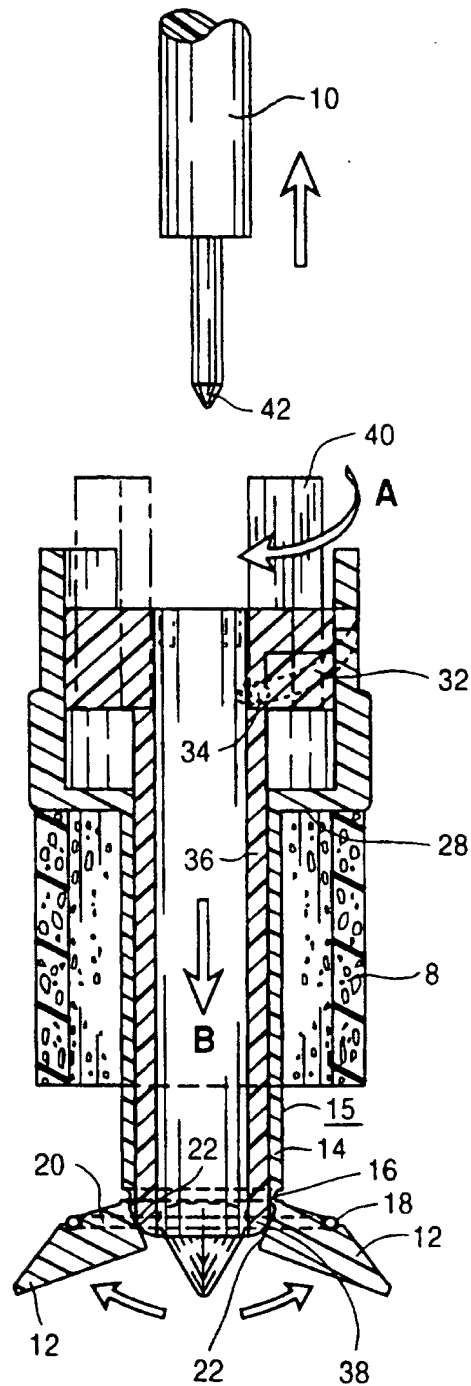**FIG. 3**

4 / 11

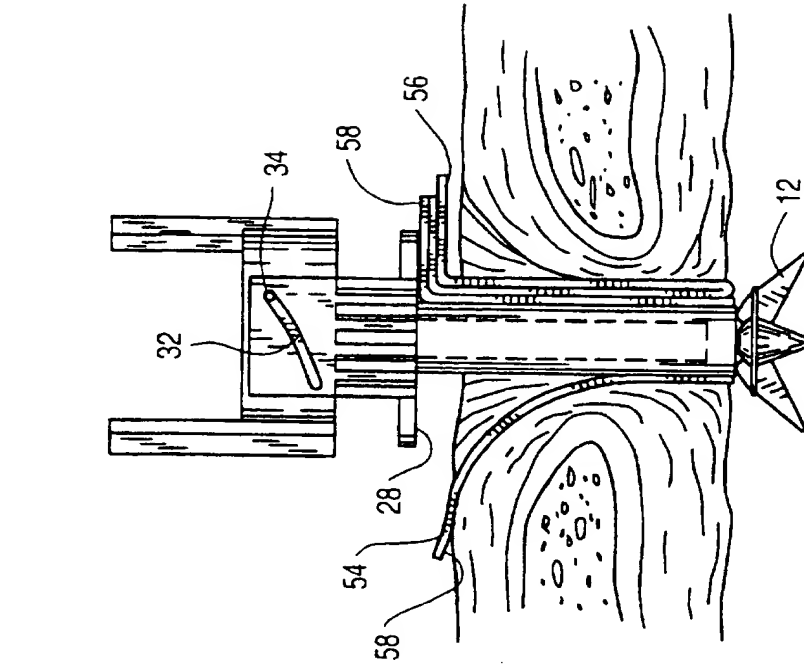


FIG. 5

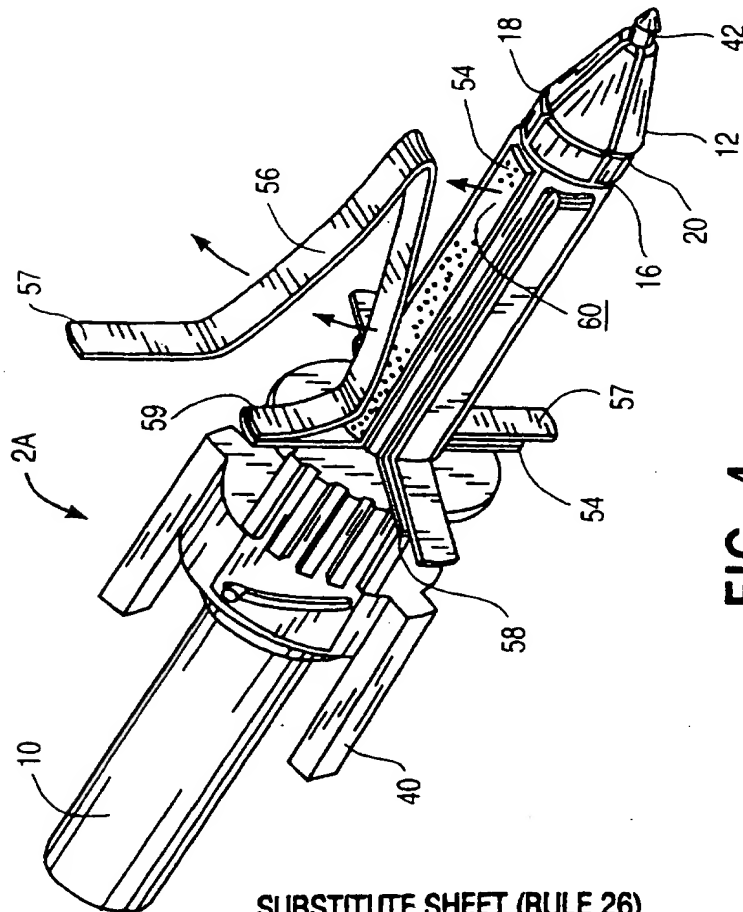


FIG. 4

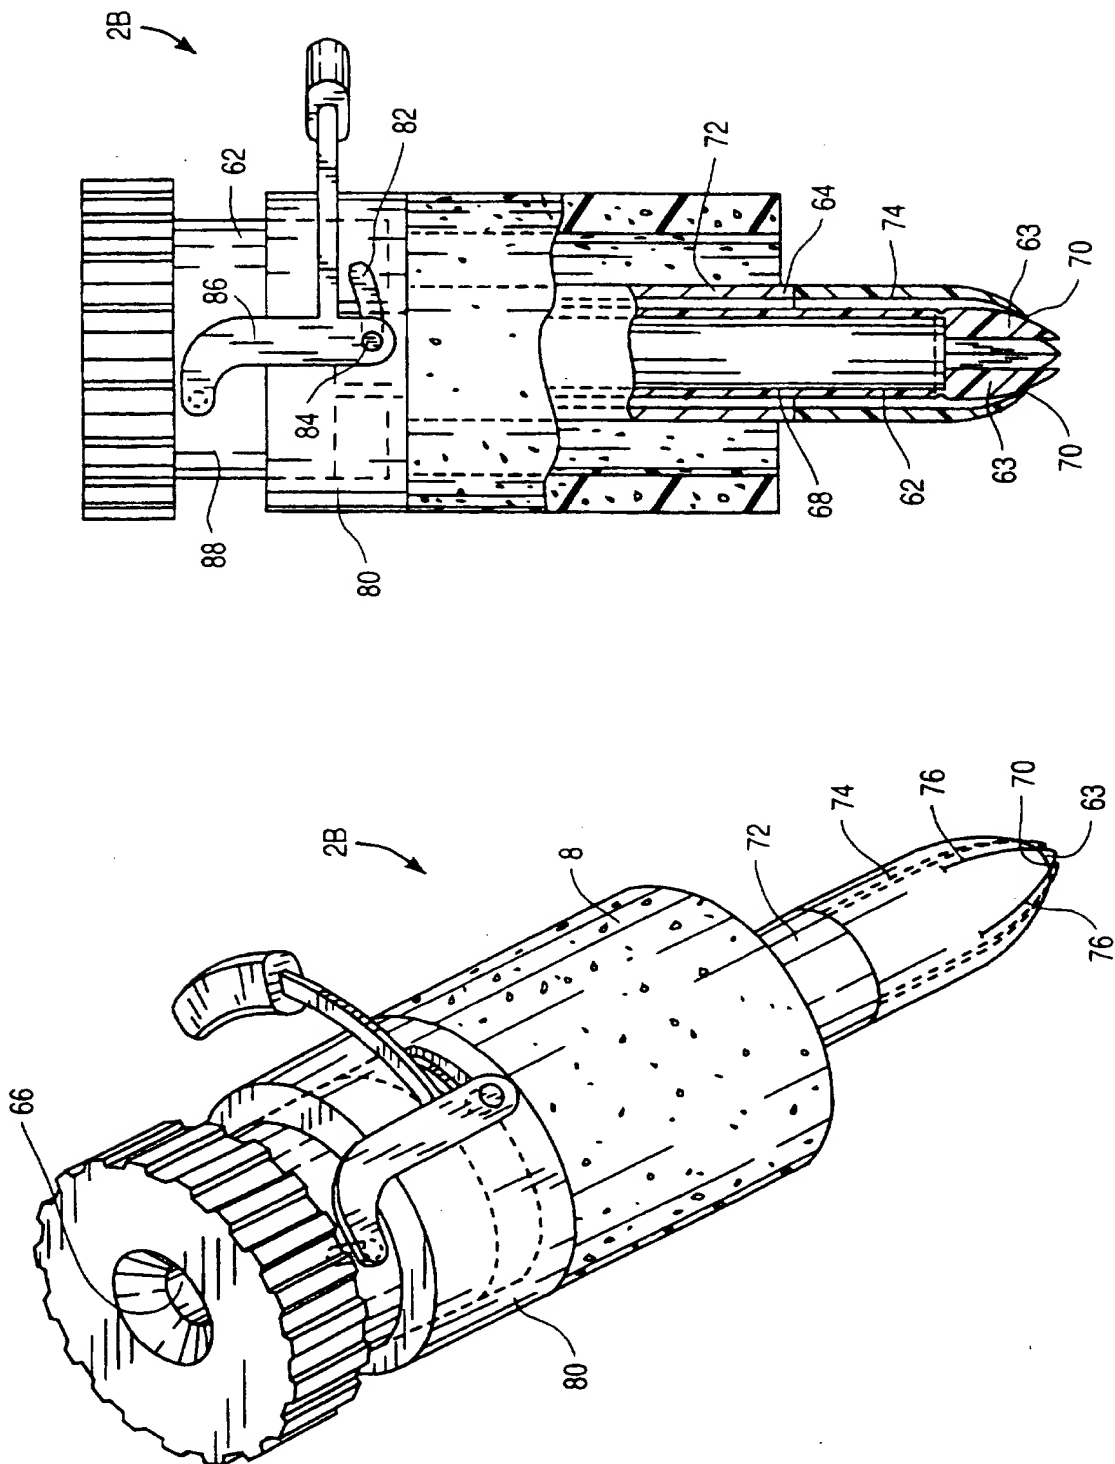


FIG. 7

FIG. 6

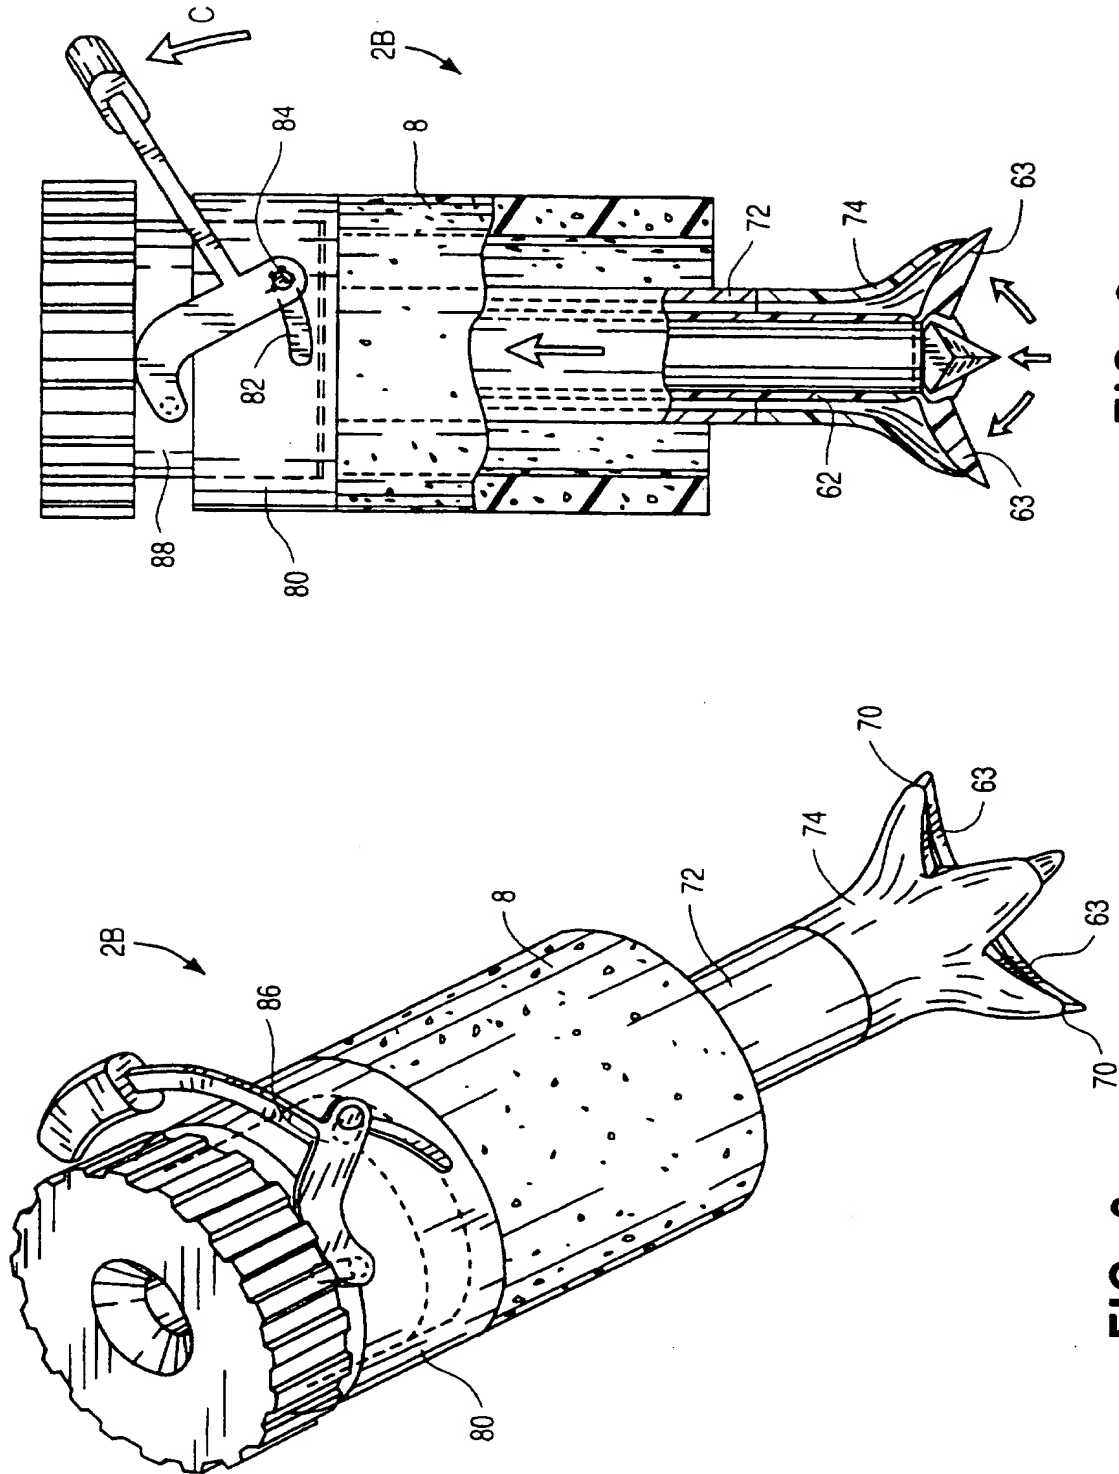


FIG. 9

FIG. 8

7/11

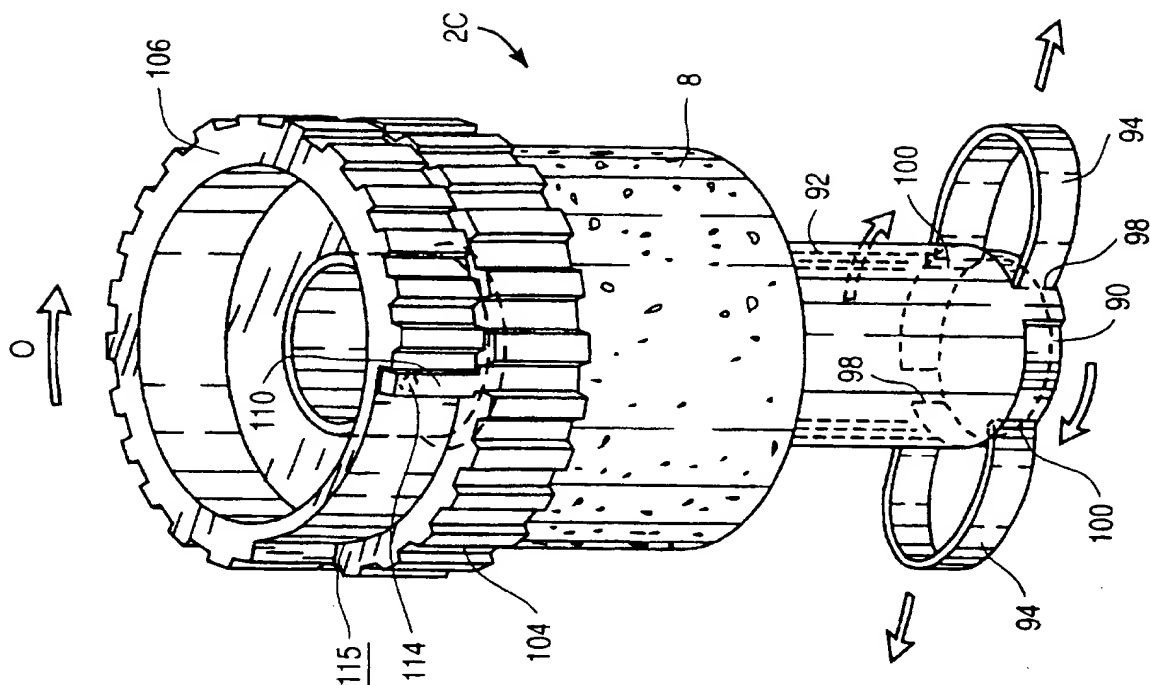


FIG. 11

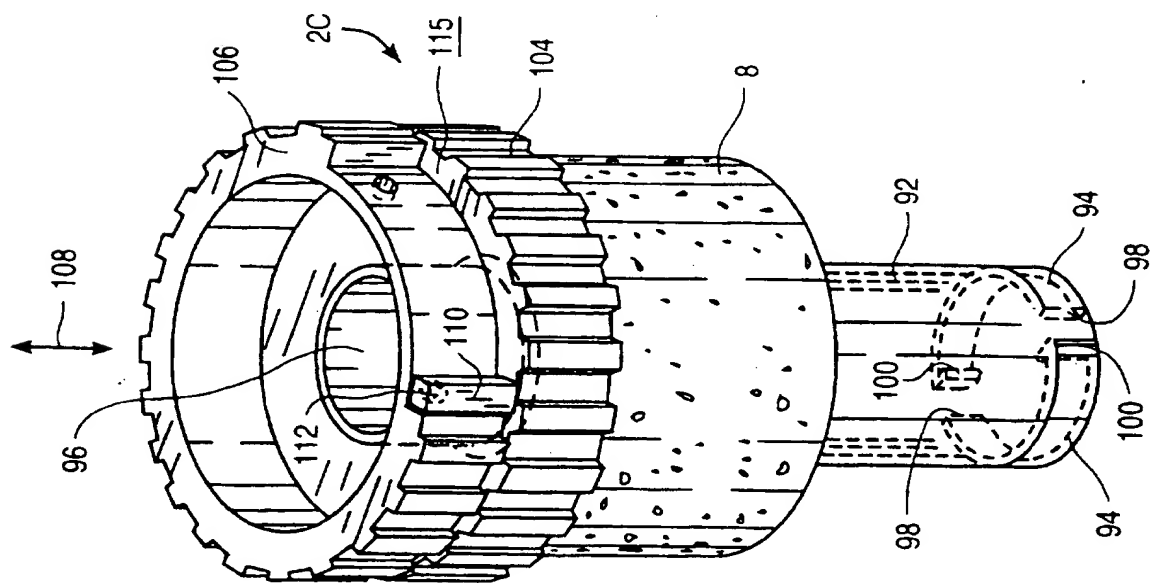


FIG. 10

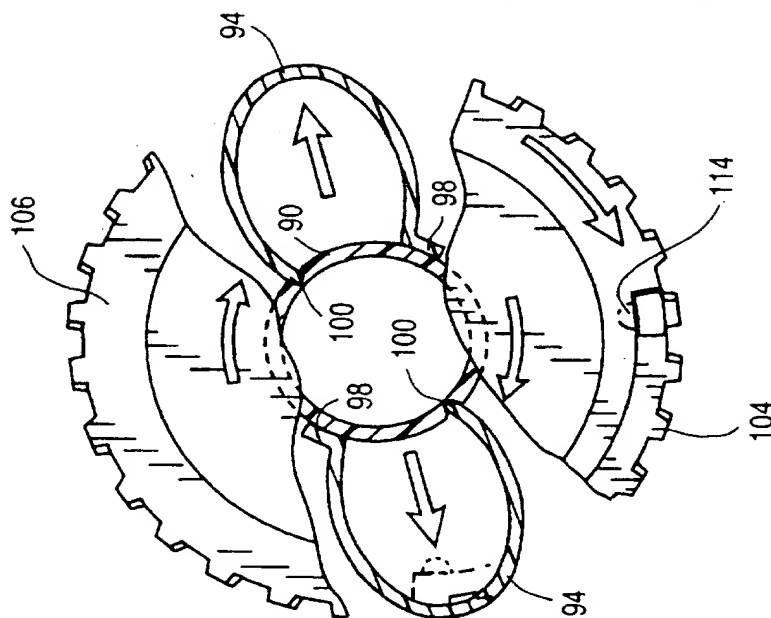


FIG. 13

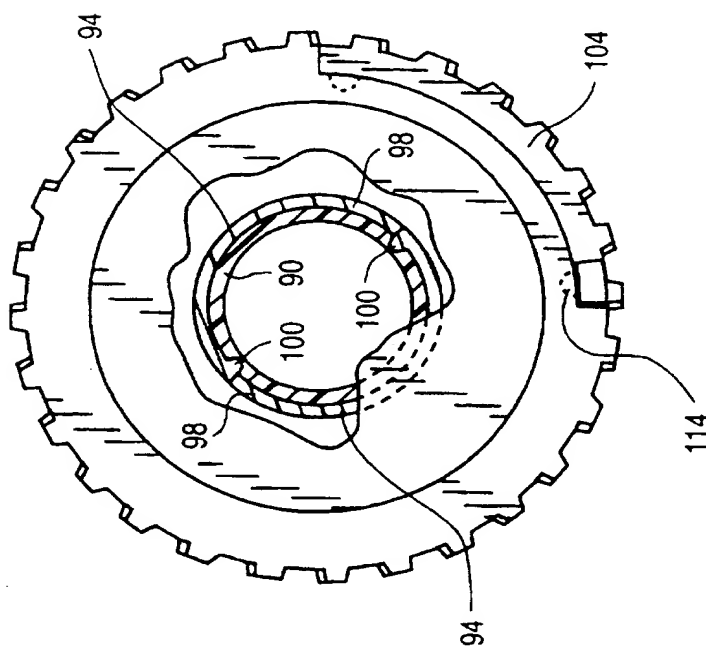


FIG. 12

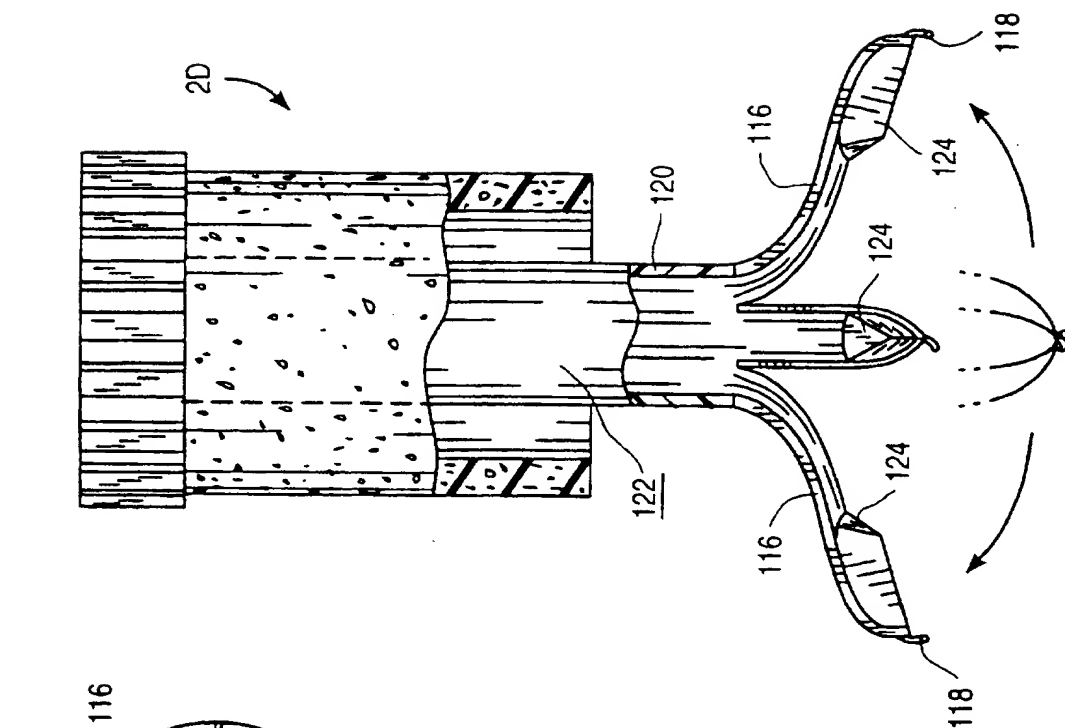


FIG. 15

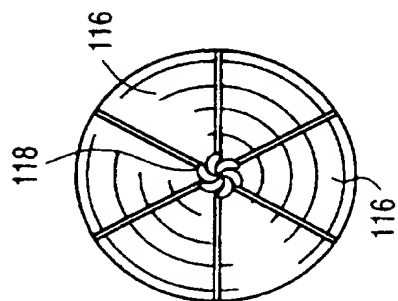


FIG. 16

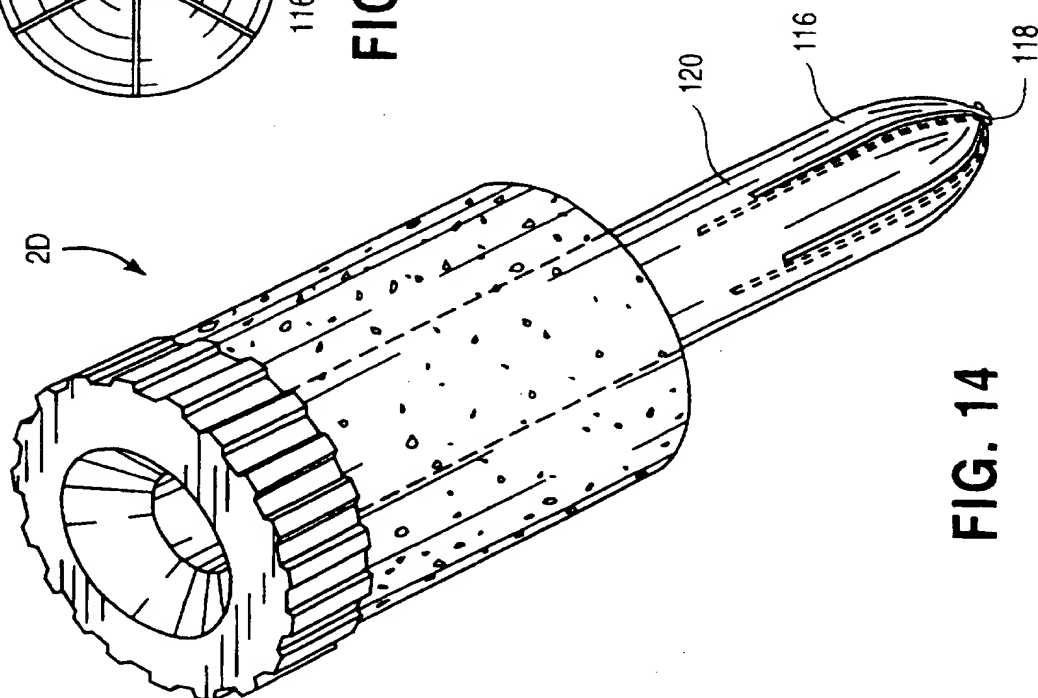


FIG. 14

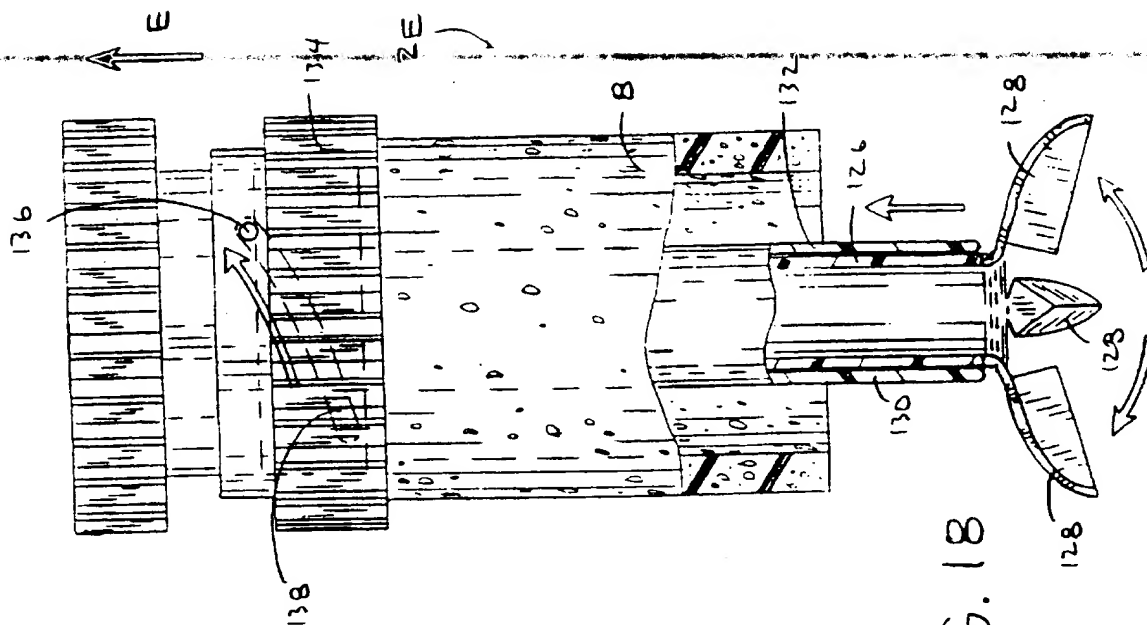


FIG. 18

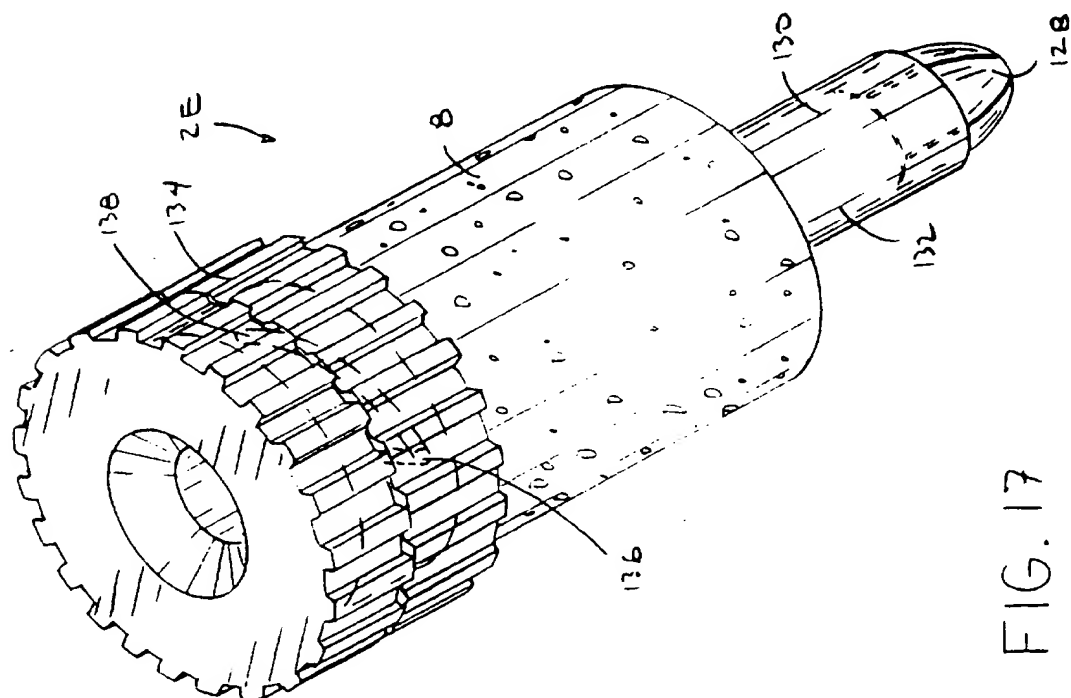
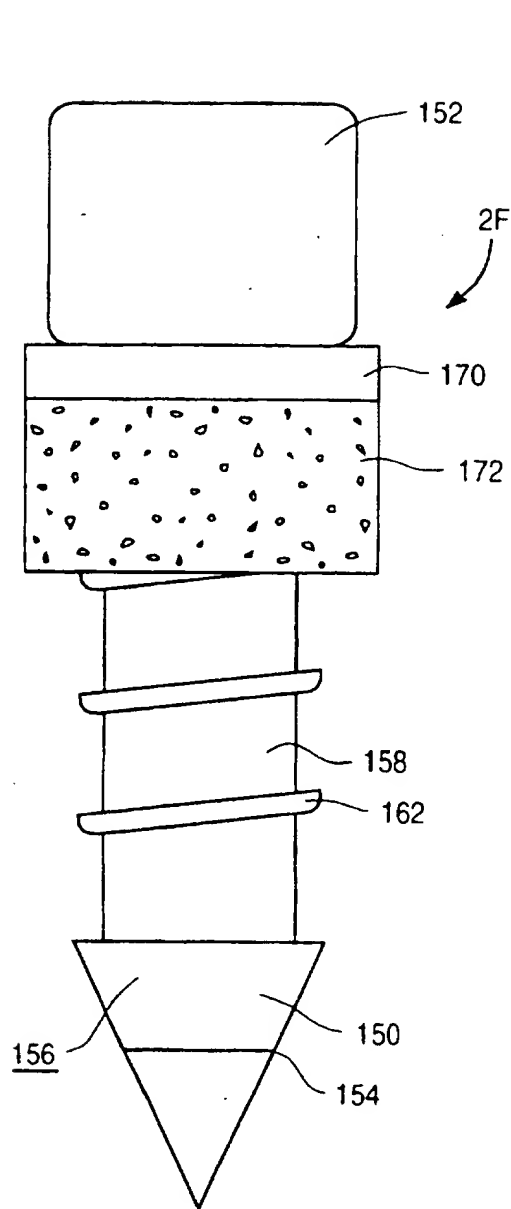
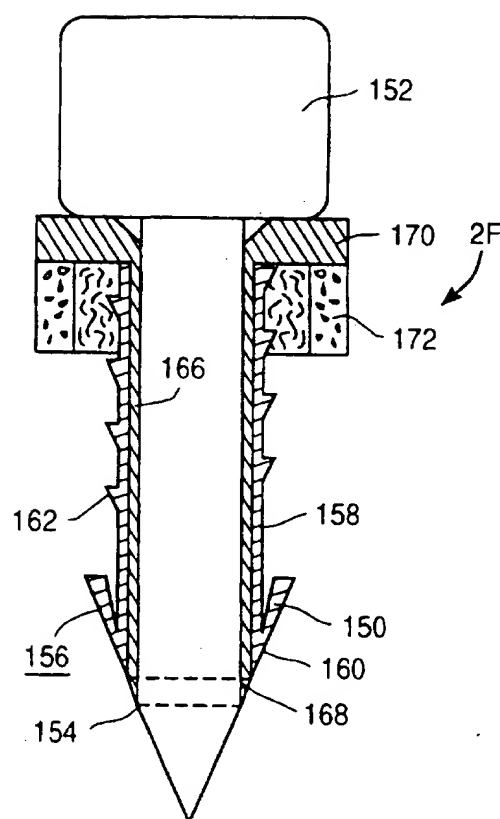


FIG. 17

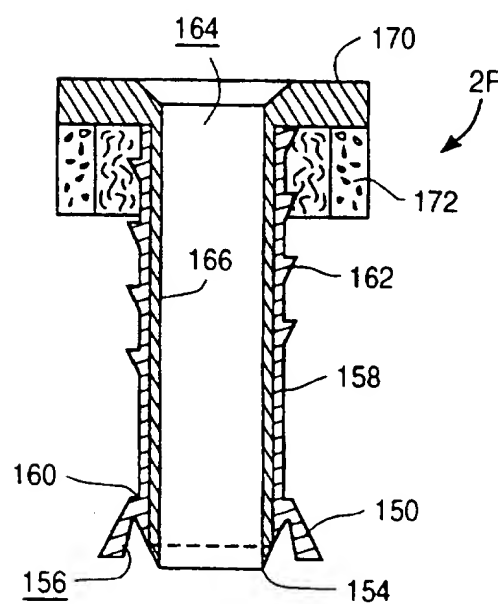




**FIG. 19**



**FIG. 20**



**FIG. 21**

## INTERNATIONAL SEARCH REPORT

International application No.  
PCT/US97/04210

## A. CLASSIFICATION OF SUBJECT MATTER

IPC(6) : A61B 17/00

US CL : 604/164

According to International Patent Classification (IPC) or to both national classification and IPC

## B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 604/105, 109, 164, 167, 174

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

## C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X	US 3,717,151 A (COLLETT) 20 February 1973, entire reference.	1-26
X	US 5,122,122 A (ALLGOOD) 16 June 1992, see entire reference .	1-26

☐ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

* Special categories of cited documents:	* "T" later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
* "A" document defining the general state of the art which is not considered to be of particular relevance	* "X" document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
* "E" earlier document published on or after the international filing date	* "Y" document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
* "L" document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	* "&" document member of the same patent family
* "O" document referring to an oral disclosure, use, exhibition or other means	
* "P" document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search

11 JULY 1997

Date of mailing of the international search report

15 AUG 1997

Name and mailing address of the ISA/US  
Commissioner of Patents and Trademarks  
Box PCT  
Washington, D.C. 20231

Authorized officer

SAM RIMELL

Facsimile No. (703) 305-3230

Telephone No. (703) 308-2677